



ELECTRONIC NOSE FOR THE CONTINUOUS MEASUREMENT OF ODOUR CONCENTRATION AT EMISSIONS: INSTRUMENT DEVELOPMENT, TRAINING AND APPLICATION

Extended abstract

**Licina Dentoni¹, Lidia Eusebio¹, Laura Capelli¹, Selena Sironi¹, Massimiliano Il Grande²,
Andrea Nicola Rossi², Marco Remondini³**

¹Politecnico di Milano, Department of Chemistry, Materials and Chemical Engineering "Giulio Natta",
Piazza L. da Vinci 32, 20133, Milano, Italy

²Progress S.r.l., via N.A. Porpora 147, 20131, Milano, Italy

³SACMI s.c., via Selice Provinciale 17/A, Imola, Italy

Background

The presence of odour in ambient air is nowadays recognized as an environmental stressor that negatively affects the quality of life (Blanes-Vidal et al., 2012). In order to evaluate odour exposure at receptors, several methods can be applied. Different regulations provide to use dispersion modelling to simulate how odour disperses into the atmosphere, and consequently to calculate hourly ground odour concentration values in the simulation space-time domain (Cusano et al., 2010). Given that a detailed characterization of emissions over time would require frequently repeated olfactometric tests, thus resulting in a very expensive (in terms of money and time) approach, emission data employed as model inputs are usually represented by averaged odour emission rate values. This approach may provide a good description of the average odour impact, but doesn't take account of fluctuations that are typical of some emission typologies (Isaac-Ho Tin Noe et al., 2010). This study discusses the possibility of installing an electronic nose directly at an emission, in order to measure odour concentration continuously and therefore to obtain data that could be possibly used as real-time inputs for dispersion models as well as hourly data to use instead of averaged values. Such an application requires the development of a specific instrument, as well as a specific training. An EOS 507 electronic nose, developed in collaboration with Sacmi s.c. and Progress S.r.l., was used to evaluate the possibility to monitor the odour concentration at the emission of a plant for hospital waste treatment.

Laboratory tests were conducted to evaluate the electronic nose capability of quantifying odour concentration: samples containing pure compounds and mixtures were tested at different concentrations, as well as real samples collected directly from the odour source.

Methods

1. The EOS 507 electronic nose

The electronic nose used for this work is an EOS 507 (Dentoni et al., 2012).

The instrument has two inlets for air: one of them is connected with the system for the neutral air realization; the other one is connected with an electronic valve that regulates the sample flow that is sent to the sensor chamber, which contains 6 MOS sensors.

Moreover, the electronic nose is equipped with a temperature and humidity sensor. For the regulation of the sample humidity, the electronic nose regulates neutral air humidity to a certain value RH_{wk} that the software calculates from the external humidity value (RH_{ext}).

With the EOS 507, only one feature is calculated from the response of each sensor, defined as E.U. (EOS Unit). All measures are normalized using an internal standard consisting of n-butanol at a known and constant

concentration and, as a consequence of this normalization, sensors responses in terms of E.U. should increase linearly with the concentration of the analyzed sample. The classification and quantification algorithm is a modified KNN-algorithm.

The electronic nose is trained with samples collected on the source to be monitored, diluted as to obtain samples at different concentrations. For sample recognition, the system compares the distance, in the 6-dimensional response space (6 sensors giving each 1 E.U. value), of the point relevant to the unknown measure to be classified and the broken lines between two neighbouring points belonging to the same olfactory class. The unknown measure is then classified as belonging to the olfactory class for which the minimum distance is measured. The odour concentration of the analysed sample is then calculated based on the odour concentrations of the points at the extremities of the segment, by evaluating the relative distance between the two points at known concentration and the position of the projection of the point representing the unknown measure.

2. Considered emission

The emission considered in this study is a chimney of a hospital waste treatment plant. More in detail, the chimney emits the air sucked from the grinder where the medical waste is first treated, as well as all the vents coming from the sterilization process. The plant operates with cycles and each cycle can be considered as composed by different phases. After collection, the medical waste is grinded and sent to a batch sterilizer. When the waste loading in the sterilizer is completed, the air inside the sterilizer is sucked by means of a pump and emitted through the chimney. After that, the sterilization process starts with the injection of steam. After 15-20 minutes, the sterilizer is vented, and this vent is emitted through the chimney, as well. The emission from the chimney is therefore variable. Based on the above described process, three different emissions typologies can be identified: the air sucked from the grinder, the vent of the air sucked from the sterilization system before the steam injection and the vent after the sterilization process. Gaseous samples were collected at the emission during these three different phases, and then tested by dynamic olfactometry in order to evaluate their odour concentration. Moreover, chemical analyses were carried out in order to determine the chemical composition of the emission.

3. Tests with pure compounds

Pure compounds to be used for laboratory tests were chosen among compounds detected in the emission. More in detail, starting from chemical analysis results, and considering the odour threshold of each compound, the theoretical odour concentration related to each single compound in the emission was estimated. Laboratory tests were conducted using those chemical compounds having the major theoretical odour concentration in the emission: ethanol and ammonia.

Gaseous samples of each pure compound were analyzed with the electronic nose at different concentrations in order to train the electronic nose to estimate odour concentration. After the training phase, gaseous samples were analysed with the EOS 507, which estimated their odour concentration. Tests were performed using gaseous samples containing ammonia and ethanol separately, as well as mixtures of the two compounds. The odour concentration of analysed samples was in the range between 20 and 500 ou_E m⁻³.

4. Tests with real samples

Different samples were collected at the emission during the 3 different phases of the process. All samples were analysed by dynamic olfactometry to determine their odour concentration. The electronic nose was trained with all real samples at different odour concentrations, between 10 and 100% of the measured odour concentration. The capability of the electronic nose to estimate the odour concentration of real samples was tested. For this purpose, different samples having different odour concentrations were obtained from collected real samples. Those samples were then analysed with EOS 507 and the estimated odour concentration registered. During the quantification process different training datasets were taken into account. First, for each odour typology, only the relevant training dataset was considered; second, a training dataset comprising all measures performed with the different odour typologies was created and used for odour quantification. The estimated and real odour concentrations were compared, to evaluate the performances of the instrument.

Results and discussion

1. Tests with pure compounds – results

Electronic nose responses to different odour concentrations of the different considered pure compounds were evaluated in order to verify the linearity between electronic nose responses (E.U.) and odour concentration. As an example, the electronic nose responses to different odour concentrations of a gaseous sample containing ethanol are reported in

Fig. 1.

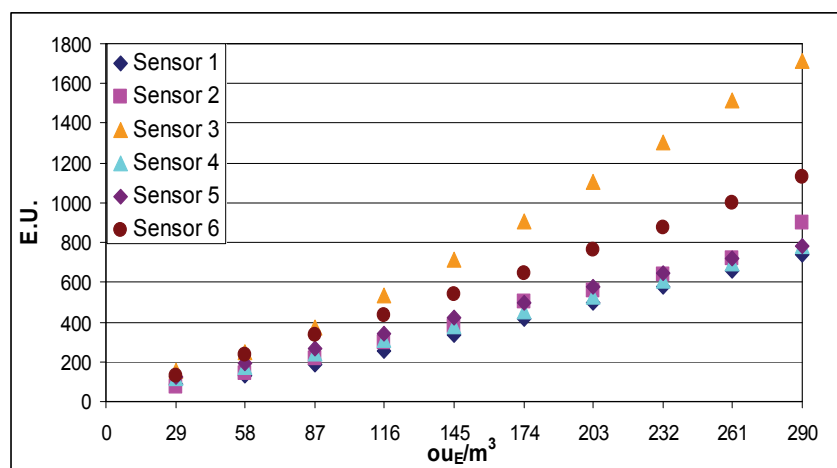


Fig. 1. E.U. registered for different odour concentrations of the ethanol sample

Some of the results of the odour concentration estimation performed by the electronic nose using the pure compounds are reported in Table 1.

In the table, the real and the estimated odour concentrations are listed; the error (per cent) of the concentration estimation is reported, as well.

Table 1. Real and estimated odour concentrations relevant to the tests with pure compounds

Tested Compound	Real concentration [$ou_E m^{-3}$]	Estimated concentration [$ou_E m^{-3}$]	Error [%]
Ethanol	145	150	3
Ethanol	145	149	3
Ethanol	290	255	12
Ethanol	290	255	12
Ethanol	290	283	2
Ethanol	290	275	5
Ethanol	580	593	2
Ammonia	82	99	21
Ammonia	164	141	14
Ammonia	246	208	15
Ammonia	328	301	8
Ammonia	411	417	1
Ammonia + Ethanol	62	70	13
Ammonia + Ethanol	125	118	6
Ammonia + Ethanol	187	194	4
Ammonia + Ethanol	249	260	4
Ammonia + Ethanol	312	306	2
Ammonia + Ethanol	124	120	3
Ammonia + Ethanol	187	193	3
Ammonia + Ethanol	312	314	1

Odour concentrations estimated by the electronic nose are comparable with the real concentration evaluated by means of dynamic olfactometry, or obtained by diluting gaseous samples having a known odour concentration. The per cent error is comprised between 1 and 20 %, and the error decreases when the odour concentration increases.

2. Tests with real samples – results

Fig. 2 reports the results obtained with the real samples. More in detail, the real odour concentration, the odour concentration estimated using only the training data set of the same emission phase (single training dataset) and the odour concentration estimated using the complete training dataset are reported.

The electronic nose is able to estimate the odour concentration of real samples with an error between 2 and 37%. The quantification system guarantees the same performances both using the single training and the complete training. In general, it can be observed that the odour concentrations estimated by the electronic nose are almost always lower than the odour concentration measured by dynamic olfactometry.

This may be due to the losses through the sampling bags that may occur during the time interval between the two analyses (Hansen et al., 2011).

Emission typology	Real concentration [ou _E m ⁻³]	Estimated concentration (single training) [ou _E m ⁻³]	Error [%]	Estimated concentration (complete training) [ou _E m ⁻³]	Error [%]
Grinding	900	600	33	599	33
Grinding	1200	843	30	839	30
Grinding	1500	1088	27	1081	28
Pre-sterilization	80	58	28	58	28
Pre-sterilization	160	101	37	101	37
Pre-sterilization	240	154	36	153	36
Pre-sterilization	320	268	16	271	15
Pre-sterilization	400	321	20	321	20
Post-sterilization	620	619	0	650	5
Post-sterilization	1240	995	20	947	24
Post-sterilization	1860	1823	2	1700	9
Post-sterilization	2480	2716	10	2656	7
Post-sterilization	3100	3921	26	3049	2

Fig. 2. Real and estimated odour concentrations relevant to the tests with real samples

Concluding remarks

Laboratory tests show that the EOS 507 is able to quantify the odour concentration of samples of pure compounds and of real samples.

The error obtained with pure compounds is comprised between 1 and 20%. The capability of the system to estimate the odour concentration turned out not to be influenced by the use of mixtures of different pure compounds in air instead of gaseous samples of pure compounds in air.

Tests performed with real samples demonstrate that the system is capable to estimate the odour concentration with the same accuracy using only a training dataset obtained with samples belonging to the same olfactory class as the sample to be quantified, as well as using a “complete” dataset, which contains data relevant to different olfactory classes. This of course is important information, meaning that the use of one single “complete” dataset will be sufficient in order to quantify the odour concentration of the monitored emission during all the phases within a satisfying level. The error relevant to the odour concentration estimation of real samples is comprised between 2 and 37%.

Laboratory tests proved the electronic nose EOS 507 to be able to quantify odour concentration with a error below 40%. Future studies will be carried out in order to verify the electronic nose performances directly in the field. Moreover, the instrument will be tested with different samples, collected on other odour sources, in order to evaluate its performances with different emissions.

Keywords: electronic nose, MOS sensors, odour emission, odour monitoring

References

- Blanes-Vidal V., Nadimi E.S., Ellermann T., Andersen H.V., Loftrom P., (2012), Perceived annoyance from environmental odors and association with atmospheric ammonia levels in non-urban residential communities: a cross-sectional study, *Environmental Health*, **11**, DOI: 10.1186/1476-069X-11-27.
- Cusano G., Licotti C., Sironi S., Capelli L., Rossi A.N. and Il Grande M., (2010), Odour regulation in Italy: the regional guidelines on odour emissions in Lombardia, *Chemical Engineering Transactions*, **23**, 19-24.
- Dentoni L., Capelli L., Sironi S., Del Rosso R., Zanetti S. and Della Torre M., (2012), Development of an electronic nose for environmental odour monitoring, *Sensors*, **12**, 14363-14381.
- Hansen M.J., Adamsen A.P.S., Feilberg A., Jonassen K.E.N. (2011), Stability of odorants from pig production in sampling bags for olfactometry, *Journal of Environmental Quality*, **40**, 1096-1102.
- Isaac-Ho Tin Noe I., Siino F., Bara C., Urvoy Y., Haaser C., Tripathi A., Ait Hamou L. and Mailliard T., (2010), Tool for predicting and monitoring the impact of wastewater treatment plants on odour, *Chemical Engineering Transactions*, **23**, 267-272.